

Introduction

Copper Mountain Technologies produces lab-grade VNAs with outstanding measurement accuracy. As with every VNA, performing a good calibration is necessary for maximizing the accuracy of VNA measurement results, for de-embedding the effects of imperfect cables and components in the fixture, and for moving the reference plane to the DUT interfaces. There are several approaches for determination and application of VNA measurement corrections, including port extension (a relatively crude, approximate method), fixture de-embedding (with accuracy depending on correctness of the model), and calibrating with a calibration kit (a high accuracy approach).

Generally, there are two broad categories of calibration kit types: traditional mechanical kits and automatic/electronic calibration modules. Within mechanical kits, there are two types of kits: those with standard “polynomial” coefficients and those with full S-parameter characterization data, also known as databased kits.

This application note introduces databased calibration kits, explains why their use is growing in popularity, and describes how they can be used with Copper Mountain Technologies VNAs.

What is a databased calibration kit?

Unlike coefficient-based mechanical kits, all of which are normally supplied with the same set of coefficients, a databased calibration kit includes a measured result of each individual standard in each kit produced. The goal when manufacturing a traditional calibration kit is trying to be as close to a mechanical and electrical specification as possible during fabrication and relies on this consistency to achieve a good accuracy with a standard set of coefficients.


In contrast, each standard in a databased calibration kit is very precisely characterized after fabrication; the measured data is supplied with the kit and, when subsequently used in the VNA for calibration, provides outstanding measurement accuracy. The advantage of databased calibration kits is such kits can achieve a similar or superior accuracy compared with traditional kits, at a lower cost to manufacture. Databased kits are starting to become more popular in recent years, as users have begun to recognize the high quality of measurement they can provide, at a relatively low cost.

Both types of calibration kit are supported by modern VNAs, thanks to significant increases in the memory and computational resources available to instruments. All Copper Mountain Technologies VNAs support databased calibration kits.

In a databased calibration kit, you will find the characterization data for each standard, which is normally supplied as touchstone, probably on a USB thumb drive. The data corresponds to that particular serial

number of calibration kit. Vendors supplying databased kits now include Keysight, Rosenberger, and Spinner among others.

Here is a picture comparing a traditional, coefficient-based calibration kit with a databased calibration kit:

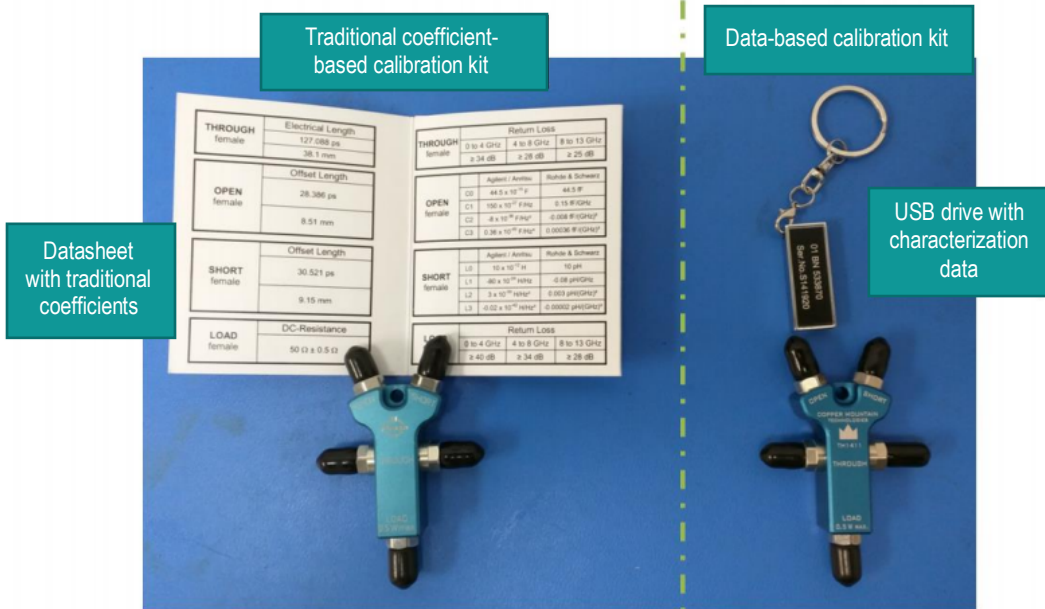

Tables of data corresponding to a traditional kit and databased kit are shown below:

Traditional coefficients for all standards

No	Type	Standard	Label	Frequency		Delay	Z0	Offset	Media	H/W	Terminal Impedance	Coefficients			
				F min	F max							C0 10 ⁻¹⁵ F	C1 10 ⁻²⁷ F ² /Hz	C2 10 ⁻³⁹ F ³ /Hz ²	C3 10 ⁻⁴⁵ F ³ /Hz ³
2	Through	Female	THROUGH	0 to 4 GHz	4 to 8 GHz	0 s	50 Ω	0	Coax		50 Ω	62.14	-143.07	82.92	0.76
5	Open	Open-M	OPEN	999 GHz	17.411 ps	0 s	50 Ω	700 MΩ/s	Coax		50 Ω	119.09	-36.955	26.258	5.5136
3	Short	Short-M	SHORT	999 GHz	17.817 ps	0 s	50 Ω	2.1002 GΩ/s	Coax		50 Ω	0	0	0	0
6	Short	Short-F	SHORT	999 GHz	93 fs	-49.992 Ω	700 MΩ/s		Coax		50 Ω	0	0	0	0
1	Load	Broadband	LOAD	999 GHz	0 s	50 Ω	700 MΩ/s		Coax		50 Ω				
7	Thru/Delay	Thru	THRU	999 GHz	0 s	50 Ω	700 MΩ/s		Coax		50 Ω				
8	Unkn Thru	Unknown Thru	THRU	999 GHz	AUTO				Coax						

A portion of the characterization data of one standard

Frequency	MLog(S11)	Arg(S11)
1475	14.75 GHz	-0.052180502 dB
1476	14.76 GHz	-0.0567747983 dB
1477	14.77 GHz	-0.0522498144 dB
1478	14.78 GHz	-0.0542020921 dB
1479	14.79 GHz	-0.0538610886 dB
1480	14.8 GHz	-0.054465739 dB
1481	14.81 GHz	-0.0565982418 dB
1482	14.82 GHz	-0.0567050339 dB
1483	14.83 GHz	-0.0565874858 dB
1484	14.84 GHz	-0.0562911521 dB
1485	14.85 GHz	-0.0588182429 dB
1486	14.86 GHz	-0.0563364984 dB
1487	14.87 GHz	-0.0572208409 dB
1488	14.88 GHz	-0.0594998903 dB
1489	14.89 GHz	-0.0562913618 dB
1490	14.9 GHz	-0.0583267663 dB
1491	14.91 GHz	-0.0552650238 dB
1492	14.92 GHz	-0.0552920788 dB
1493	14.93 GHz	-0.0549213992 dB
1494	14.94 GHz	-0.0533407817 dB
1495	14.95 GHz	-0.0516521843 dB
1496	14.96 GHz	-0.0552069151 dB
1497	14.97 GHz	-0.0536740653 dB
1498	14.98 GHz	-0.0530236532 dB
1499	14.99 GHz	-0.0517217297 dB
1500	15 GHz	-0.0558233194 dB



Defining a databased kit in VNA software

Since every databased calibration kit has a unique set of data (usually contained in a Touchstone S1P file), the calibration kit definition needs to be created for each kit. This application note is based on the software of the Copper Mountain Technologies' Planar 804/1, a 2-port VNA measuring from 100 kHz to 8.0 GHz; other instruments' software will follow a similar procedure as well.

To create the databased calibration kit definition, use the softkeys along the right side of the user interface to navigate to Calibration -> Cal Kit. Choose any empty calibration kit entry and type in a Label name. Now, choose "Define STDs". When defining the standards, standards with database—such as Short, Open and Load in this example—should be specified as databased.

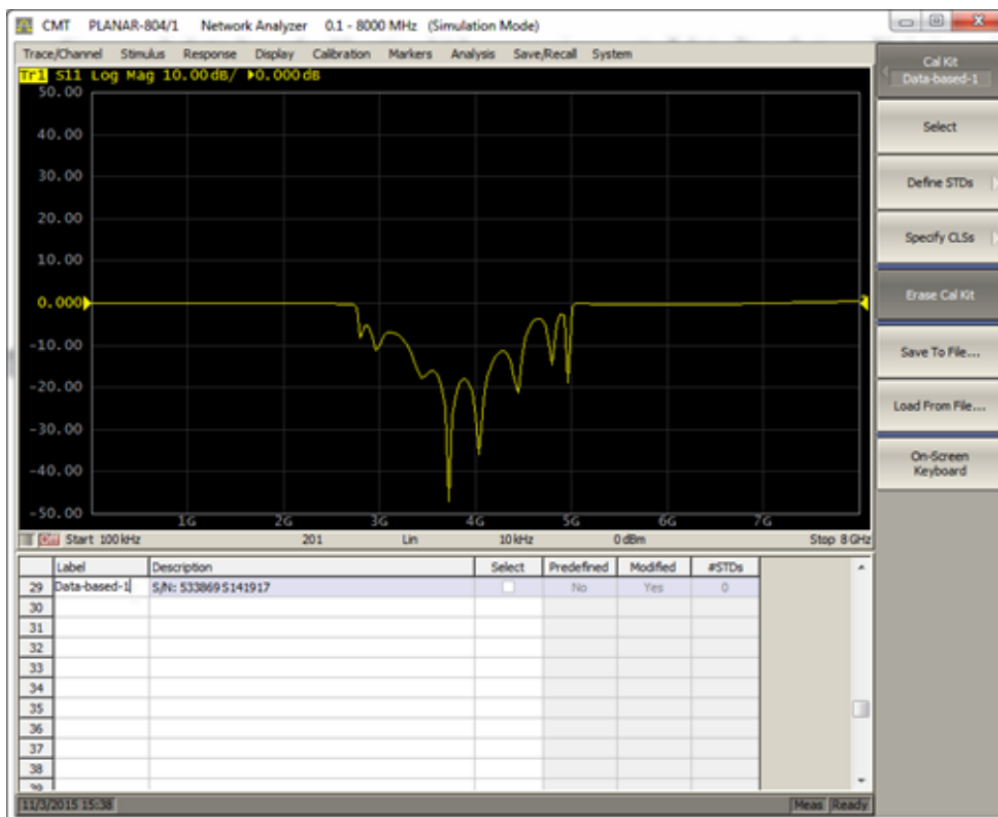


Figure 1: Choose any blank calibration kit in the table, and type the kit Name and Description.



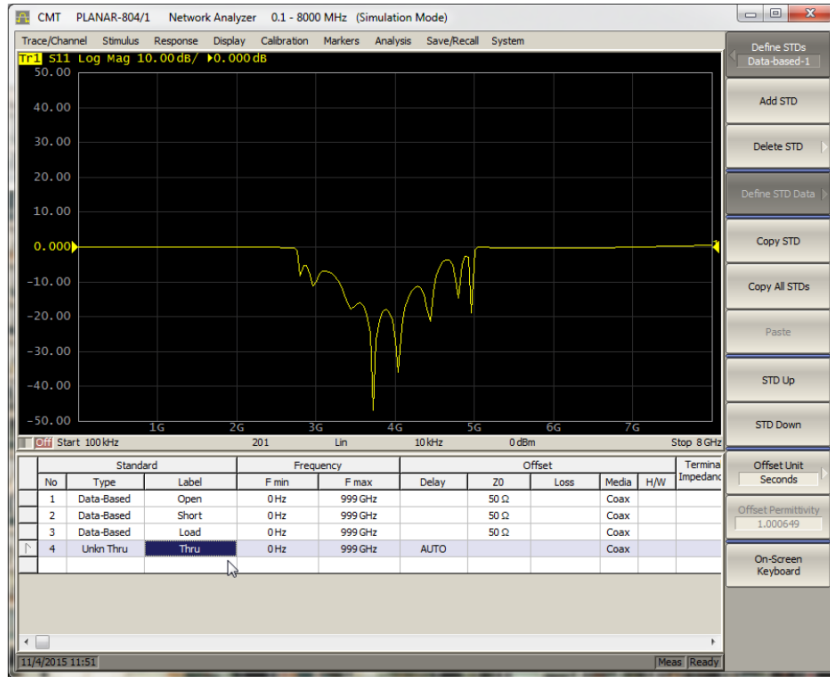


Figure 2: Create all the individual standards. Each databased standard should be specified as Type “Data-Based”.

Next, use the softkey sequence Define STD Data ⇒ Load Data From Touchstone File. Navigate to and load the Touchstone file corresponding to each standard.

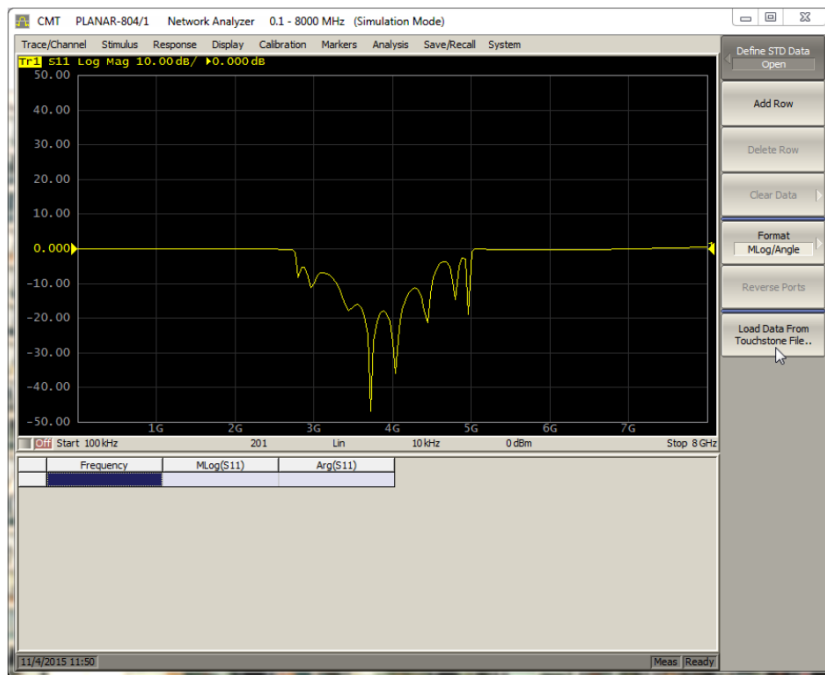


Figure 3: Loading the touchstone file supplied with the kit for each standard.



After successfully defining the standards, you also need to specify the class of each before performing the calibration. Go to Calibration ⇒ Cal Kit and select the databased kit. Then choose Specify CLS; select ports and subclasses for each standard. Enabling “Assign Same STDs To All Ports” can reduce the number of entries required when the same standards are used on all ports.

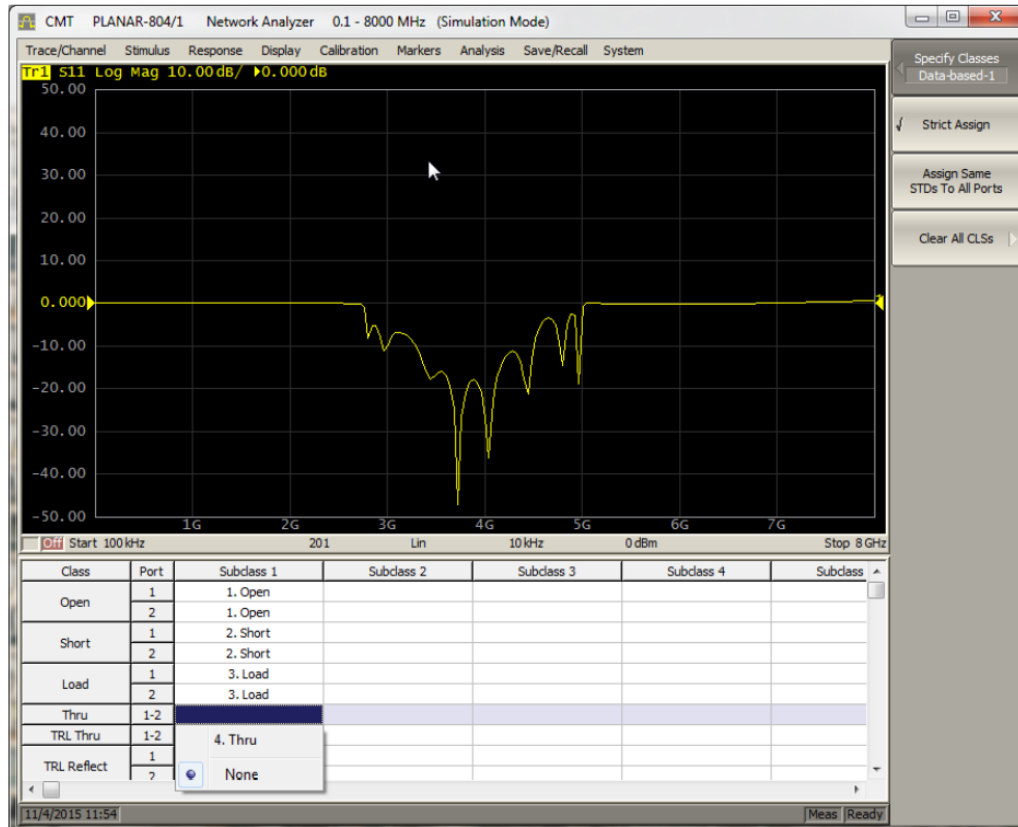


Figure 4: Specifying Classes and port scope of each standard.

Performing calibration with a databased kit

Now that the kit is defined, you are ready to perform the calibration as usual. Just select the calibration kit by using the menu sequence Calibration ⇒ Cal Kit ⇒ Select. Now perform the calibration of your choice via the sequence Calibration ⇒ Calibrate.



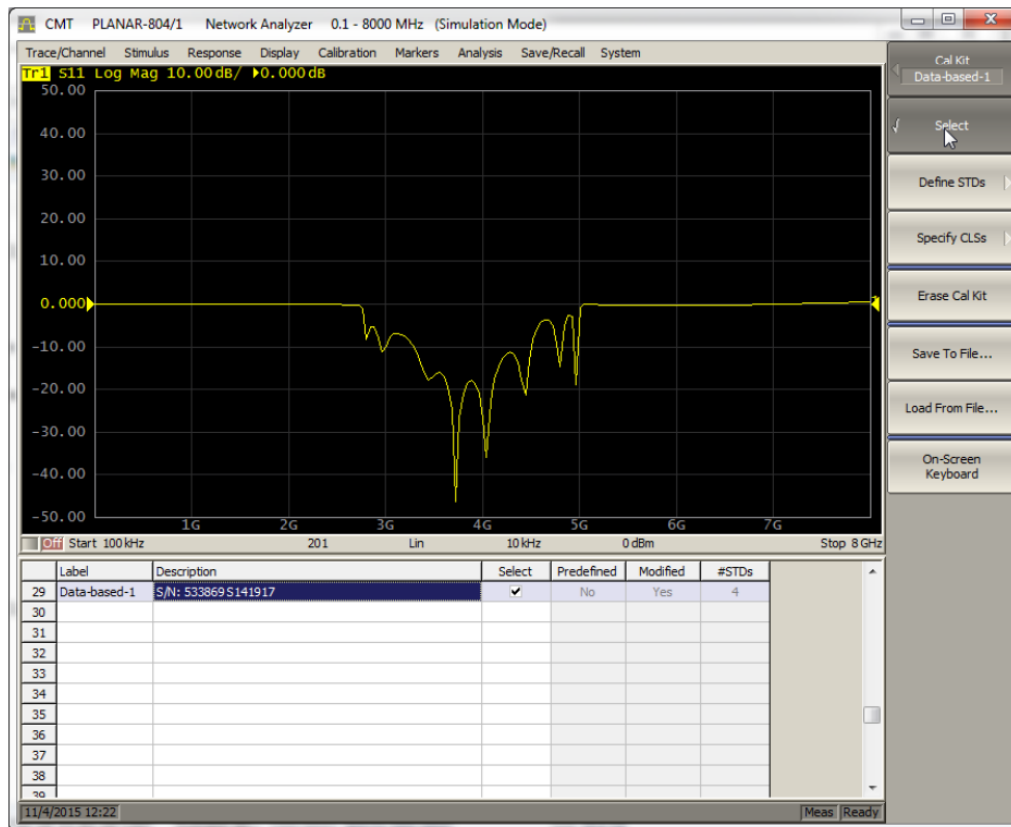


Figure 5: Selection of the calibration kit.

Conclusion

Databased calibration kits are another option for mechanical calibration kits. It's likely to be a more cost-effective solution providing similar or better accuracy of measurements compared with precision coefficient-based kits. Defining and using a databased calibration in CMT VNA software is fairly easy and straightforward. As always, if we can be of any help in your calibration or measurement solution, feel free to contact our support team at support@coppermountaintech.com.

